

ORDERING INFORMATION

THE MYNXGRIP® Vascular Closure Device includes:

(1) Balloon catheter with integrated sealant

(1) 10ml locking syringe

SIZE	COLOR	MYNX ORDER NUMBER
6F/7F	Green	MX6721
5F	Gray	MX5021

To order the MYNXGRIP® Vascular Closure Device in the United States contact your local Cordis sales rep or customer service at 800.327.7714. To learn more visit cordis.com/mynx

Rx ONLY

INDICATIONS FOR USE

The MYNXGRIP® Device is indicated for use to seal femoral arterial and femoral venous access sites while reducing times to hemostasis and ambulation in patients who have undergone diagnostic or interventional endovascular procedures utilizing a 5F, 6F or 7F procedural sheath.

PRECAUTIONS

The MYNXGRIP® Device should only be used by a trained licensed physician or healthcare professional. The MYNXGRIP® Device should not be used in patients with a known allergy to PEG.

WARNINGS

Do not use if components or packaging appear to be damaged or defective or if any portion of the packaging has been previously opened. DO NOT REUSE OR RESTERILIZE. The MYNXGRIP® Device is for single use only. The balloon catheter is loaded with a single hydrogel sealant. Reuse of the device would result in no delivery of hydrogel sealant. Do not use the MYNXGRIP® Device if the puncture site is located above the most inferior border of the inferior epigastric artery (IEA) (for arterial application) and/or above the inguinal ligament based upon osseus landmarks,

since such a puncture site may result in a retroperitoneal hematoma/bleed. Perform a femoral angiogram or venogram to verify the location of the puncture site. Do not use the MYNXGRIP® Device if the puncture is through the posterior wall or if there are multiple punctures, as such punctures may result in a retroperitoneal hematoma/bleed.



MYNXGRIP
MYNXGRIP® VASCULAR CLOSURE DEVICE

FINISH STRONG

Cordis
A Cardinal Health company

Caution: Federal (USA) law restricts these devices to sale by or on the order of a physician. For information on indications, contraindications, warnings, precautions, and adverse events, see Full Instructions for Use. For Healthcare Professional Only.

© 2016 Cardinal Health. All rights reserved. CORDIS, the Cordis LOGO, and MYNXGRIP are trademarks or registered trademarks of Cardinal Health. The MYNXGRIP® Vascular Closure Device is manufactured by Cardinal Health and is part of the Cordis portfolio. MKT7782.E 11/16

Cordis
A Cardinal Health company



REMOVE DEVICE

- Hold the MYNXGRIP® Vascular Closure Device by the shuttle while removing from the tray



PREPARE BALLOON

- Fill locking syringe with 2-3ml of sterile saline
- Attach to stopcock and draw vacuum
- Inflate balloon until black marker on inflation indicator is fully visible
- Deflate balloon and leave syringe at neutral
- Do not remove sealant sleeve

STEP 1: ACHIEVE TEMPORARY HEMOSTASIS

INSERT DEVICE



Insert the MYNXGRIP® Device into existing procedural sheath up to the white shaft marker

INFLATE THE BALLOON



Inflate the balloon until the black marker is fully visible on the inflation indicator and close stopcock

GENTLY PULL BACK TWO STOPS



- Grasp black handle and withdraw catheter until the balloon abuts the distal tip of the procedural sheath (first point of resistance)
- Continue to withdraw until the balloon abuts the arteriotomy site (second point of resistance)
- While holding adequate tension on device handle, open stopcock on procedural sheath

RESULT

CONFIRM POSITION AT THE ARTERIOTOMY




STEP 2: PLACE THE SEALANT

ADVANCE THE SEALANT




With stopcock open, detach shuttle and advance until resistance is felt

UNSHEATH THE SEALANT

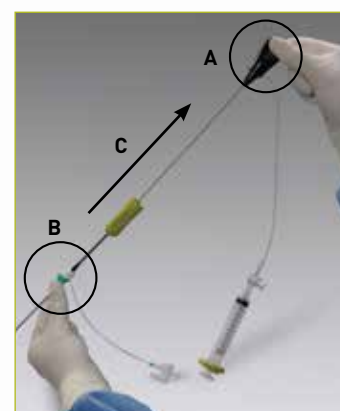

- A.** Lighten hold on black handle
- B.** Grasp procedural sheath and withdraw it from tissue tract
- C.** Continue retracting until shuttle locks onto black handle

ADVANCE PAST SINGLE GREEN MARK

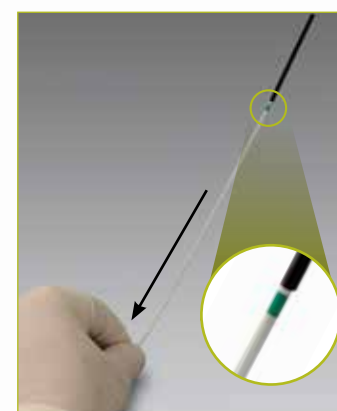

- Ensure adequate tension is employed on the black handle to keep balloon abutted against the arteriotomy
- Immediately grasp advancer tube at skin and gently advance until single marker is fully visible
- Hold for up to 30 seconds
- Lay device down for up to 90 seconds

RESULT

SEALANT IS IN PLACE



STEP 3: REMOVE THE DEVICE

LOCK, STABILIZE, DEFLATE



LOCK SYRINGE

- Lock syringe to maximum negative position



STABILIZE ARTERY

- Stabilize by applying light fingertip compression proximal to the insertion site
- Lightly grasp advancer tube at skin with thumb and forefinger; realign with tissue tract



DEFLATE THE BALLOON

- Open stopcock to deflate balloon
- To ensure complete balloon deflation, wait until air bubbles and fluid have stopped moving through the inflation tubing

REMOVE



REMOVE CATHETER AND ADVANCER TUBE

- Withdraw catheter through the advancer tube lumen
- NOTE:** If unusual resistance is felt during catheter withdrawal, pull the advancer tube and balloon catheter together through the tissue tract
- Remove advancer tube from the tissue tract

RESULT

SECURE EXTRAVASCULAR CLOSURE

